



**Safety instructions**  
**FIBERTRAC 31, 32**  
**SOLITRAC 31**  
**MINITRAC 31, 32**  
**POINTRAC 31**  
**WEIGHTRAC 31, 32**

Flameproof enclosures  
Dust ignition protection by enclosure  
Intrinsic safety  
BVS 10 ATEX E 096  
Profibus PA  
Foundation Fieldbus



CE 0044



Document ID: 55440



**VEGA**

## Contents

1	Area of applicability.....	4
2	General information.....	4
3	Special instructions for installation.....	6
4	Installation, assignment zones/EPL areas.....	8
5	Safe operating mode.....	8
6	Grounding.....	8
7	Material resistance.....	8
8	Different ignition protection types.....	8
9	Electrical data.....	9
10	Thermal data.....	11
11	Protection against static electricity.....	11
12	Impact and friction sparks.....	12
13	Mounting with external display unit VEGADIS 61/81.....	12
14	Ignition protection type flameproof enclosure Ex "d".....	12
15	Ignition protection type protection by enclosure Ex "t".....	13
16	Instructions for zone 20 applications.....	14
17	Ignition protection type intrinsic safety Ex "ia".....	14
18	Use of an overvoltage arrester.....	14
19	Version with cooling option.....	15

Supplementary documentation:

- Operating Instructions FIBERTRAC 31, 32, SOLITRAC 31, MINITRAC 31, 32, POINTRAC 31, WEIGHTRAC 31, 32
- WHG Überfüllsicherung FIBERTRAC 31, SOLITRAC 31, MINITRAC 31, POINTRAC 31
- EU-type approval certificate BVS 10 ATEX E 096, Issue 02 (Document ID: 55198)
- EU declaration of conformity (Document ID: 44391)

Editing status: 2017-01-17

DE	Sicherheitshinweise für den Einsatz in explosionsgefährdeten Bereichen
EN	Safety instructions for the use in hazardous areas
FR	Consignes de sécurité pour une application en atmosphères explosibles
IT	Normative di sicurezza per l'impiego in luoghi con pericolo di esplosione
ES	Instrucciones de seguridad para el empleo en áreas con riesgo de explosión
PT	Normas de segurança para utilização em zonas sujeitas a explosão
NL	Veiligheidsaanwijzingen voor gebruik op plaatsen waar ontploffingsgevaar kan heersen
SV	Säkerhetsanvisningar för användning i explosionsfarliga områden
DA	Sikkerhedsforskrifter til anvendelse i explosionsfarlig atmosfære
FI	Turvallisuusohjeet räjähdysvaarallisissa tiloissa käyttöä varten
EL	Υποδείξεις ασφαλείας για τη χρησιμοποίηση σε περιοχές που υπάρχει κίνδυνος έκρηξης

DE	Die vorliegenden Sicherheitshinweise sind im Download unter <a href="http://www.vega.com">www.vega.com</a> standardmäßig in den Sprachen deutsch, englisch, französisch und spanisch verfügbar. Weitere EU-Landessprachen stellt VEGA nach Anforderungen zur Verfügung.
EN	These safety instructions are available as a standard feature in the download area under <a href="http://www.vega.com">www.vega.com</a> in the languages German, English, French and Spanish. Further EU languages will be made available by VEGA upon request.
FR	Les présentes consignes de sécurité sont disponibles au téléchargement sous <a href="http://www.vega.com">www.vega.com</a> en standard en allemand, en anglais, en français et en espagnol. VEGA met à disposition d'autres langues de l'Union Européenne selon les exigences.
ES	Las indicaciones de seguridad presentes están disponibles en la zona de descarga de <a href="http://www.vega.com">www.vega.com</a> de forma estándar en los idiomas inglés, francés y español. VEGA pone a disposición otros idiomas de la UE cuando son requeridos.

## 1 Area of applicability

These safety instructions apply to the radiation-based sensors of the PROTRAC series:

FIBERTRAC FT31/2.DK\*C/D/E/G\*\*\*\*(\*)\*\*, FIBERTRAC FT31.AW\*E/G\*\*\*\*(\*)\*\*  
 SOLITRAC ST31.DK\*C/D/E/G\*\*\*\*(\*)\*\*, SOLITRAC ST31.AW\*E/G\*\*\*\*(\*)\*\*  
 MINITRAC MT31/2.DK\*C/D/E/G\*\*\*\*, MINITRAC MT31.AW\*E/G\*\*\*\*  
 POINTRAC PT31.DK\*C/D/E/G\*\*\*\*(\*)\*\*, POINTRAC PT31.AW\*E/G\*\*\*\*(\*)\*\*  
 WEIGHTRAC WT31/2.DK\*C/D/E/G\*\*\*\*\*

according to EU type approval certificate BVS 10 ATEX E 096, Issue 02 (certificate number on the type label) and for all instruments with safety instruction (55440) on the type label.

## 2 General information

The sensors of the PROTRAC series are part of the radiation-based measuring principle.

In a radiation-based measurement, a weak radioactive source on the tank emits focused gamma rays. A special detector mounted on the opposite side of the tank receives the radiation which is converted into flashes of light. The number of these flashes is detected and evaluated.

The FIBERTRAC 31, FIBERTRAC 32 and SOLITRAC 31 sensors of the PROTRAC series are suitable for non-contact level and interface measurement.

The MINITRAC 31, MINITRAC 32 sensors of the PROTRAC series are suitable for the non-contact, continuous density measurement and level detection of liquids and bulk solids in pipelines and vessels.

The POINTRAC 31 sensors of the PROTRAC series are suitable for non-contact level detection of liquids and bulk solids.

The WEIGHTRAC 31, WEIGHTRAC 32 sensors of the PROTRAC series are suitable for non-contact, continuous mass flow measurement of bulk solids on conveyor belts and screw conveyors.

The sensors of the PROTRAC series FIBERTRAC FT31/2.DK\*C/D/E/G\*\*\*\*(\*)\*\*, FIBERTRAC FT31.AW\*E/G\*\*\*\*(\*)\*\*, SOLITRAC ST31.DK\*C/D/E/G\*\*\*\*(\*)\*\*, SOLITRAC ST31.AW\*E/G\*\*\*\*(\*)\*\*, MINITRAC MT31/2.DK\*C/D/E/G\*\*\*\*, MINITRAC MT31.AW\*E/G\*\*\*\*, POINTRAC PT31.DK\*C/D/E/G\*\*\*\*(\*)\*\*, POINTRAC PT31.AW\*E/G\*\*\*\*(\*)\*\*, WEIGHTRAC WT31/2.DK\*C/D/E/G\*\*\*\*\* when used with "Flameproof enclosure (Ex d)" are suitable for the use in hazardous atmosphere of all combustible substances of explosion groups IIA, IIB and IIC, for applications requiring instruments of category 2G.

The sensors of the PROTRAC series are suitable for applications requiring category 2G (EPL Gb) instruments.

The sensors of the PROTRAC series FIBERTRAC FT31/2.DK\*C/D/E/G\*\*\*\*(\*)\*\*, FIBERTRAC FT31.AW\*E/G\*\*\*\*(\*)\*\*, SOLITRAC ST31.DK\*C/D/E/G\*\*\*\*(\*)\*\*, SOLITRAC ST31.AW\*E/G\*\*\*\*(\*)\*\*, MINITRAC MT31/2.DK\*C/D/E/G\*\*\*\*, MINITRAC MT31.AW\*E/G\*\*\*\*, POINTRAC PT31.DK\*C/D/E/G\*\*\*\*(\*)\*\*, POINTRAC PT31.AW\*E/G\*\*\*\*(\*)\*\*, WEIGHTRAC WT31/2.DK\*C/D/E/G\*\*\*\*\* when used with "Protection through housing (Ex t)" are suitable for the use in areas with combustible, dust generating bulk solids of explosion groups IIA, IIB and IIC. These sensors of the PROTRAC series are suitable for applications requiring instruments of category 1D (EPL Da) or instruments of category 2D (EPL Db).

If the PROTRAC-Serie (x)xxxTRAC xT31/2.DK\*C/D/E/G\*\*\*\*, (x)xxxxTRAC xT31.AW\*E/G\*\*\*\* are installed and operated in hazardous areas, the general Ex installation regulations EN 60079-14 as well as these safety instructions must be observed.

### Ignition protection label

EN 60079-0, EN 60079-1, EN 60079-11, EN 60079-31

II 2(1)G Ex db [ia Ga] IIC T6 Gb

II 1D Ex ta [ia Da] IIIC T98 °C Da IP 66

II 2(1)D Ex tb [ia Da] IIIC T98 °C Db IP 66

## Important specification in the type code


### PROTRAC-Serie (x)xxxxTRAC xT3\*.a\*cdef\*h(\*)

Position		Feature	Description
(x)xxxxTRAC	Device name	FIBER	FIBERTRAC FT31, FIBERTRAC FT32
		SOLI	SOLITRAC ST31
		MINI	MINITRAC MT31, MINITRAC MT32
		POIN	POINTRAC PT31
		WEIGH	WEIGHTRAC WT31, WEIGHTRAC WT32
xT3*	Instrument code	F	FIBERTRAC FT31, FIBERTRAC FT32
		S	SOLITRAC ST31
		M	MINITRAC MT31, MINITRAC MT32
		P	POINTRAC PT31
		W	WEIGHTRAC WT31, WEIGHTRAC WT32
a	Approval	DK	II 2(1)G Ex db [Ex ia Ga] IIC T6; II 1D, 2(1)D Ex ta, tb [Ex ia Da] IIIC T98°C Da, Db IP 66
		AW	II 2(1)G Ex db [Ex ia Ga] IIC T6; II 1D, 2(1)D Ex ta, tb [Ex ia Da] IIIC T98°C Da, Db IP 66 + Overfill protection (WHG)
c	Electronics	C	Four-wire, Foundation Fieldbus (Ex-d output)
		D	Four-wire, Foundation Fieldbus (Ex-ia output)
		E	Four-wire, Profibus PA (Ex-d output)
		G	Four-wire, Profibus PA (Ex-ia output)
d	Housing / Protection	D	Aluminium double chamber / IP 66/IP 67
		W	Stainless steel double chamber / IP 66/IP 67
		A	Aluminium double chamber with 316L Conduit cooling connection / IP 66/IP 67
		V	Stainless steel double chamber with 316L Conduit cooling connection / IP 66/IP 67
		S	Aluminium double chamber (special colour) / IP 66/IP 67
		R	Aluminium double chamber (special colour) with 316L Conduit cooling connection / IP 66/IP 67
e	Cable entry / Cable gland / Plug connection	M	M20 x 1.5 / without / without
		N	½ NPT / without / without

Position		Feature	Description
f	Display and adjustment module PLICSCOM	X	without
		F	without; lid with inspection window
		B	Laterally mounted
		L	laterally mounted; with Bluetooth, magnetic pen operation
		S	laterally mounted; with Bluetooth, battery, magnetic pen operation
h	Measuring length	(*)**	2 or 3-digit measuring length of the sensor connection with FIBERTRAC FT31, FIBERTRAC FT32, SOLITRAC ST31 and POINTRAC PT31  This feature is not available with MINITRAC MT31, MINITRAC MT32.
h(*)	Frame setup	***	Different features of the frame setup with frame construction, measuring width, clear height and source fastening with WEIGHTRAC WT31, WEIGHTRAC WT32

### 3 Special instructions for installation

- The following requirements must be fulfilled for mounting, electrical installation, setup and maintenance of the instrument:
  - The staff must be qualified according the respective tasks
  - The staff must be trained in explosion protection
  - The staff must be familiar with the respectively valid regulations, e.g. planning and installation acc. to EN 60079-14
- The instrument has to be mounted according to the manufacturer specifications and the valid regulations and standards.
- Modifications on the instruments can influence the explosion protection and hence the safety. Modifications must only be carried out by employees authorized by VEGA company.
- Keep in mind for instrument mounting
  - mechanical damage on the instrument must be avoided
  - mechanical friction must be avoided
- The instruments must be mounted/installed in such a way that the following can be ruled out:
  - electrostatic charges during operation, maintenance and cleaning.
  - process-related electrostatic charges, e.g. by measuring media flowing past
- Take note of the type and size of the thread
  - Label in the area of the thread with respective name.
  - Only use the cable entries and closing screws if they are required and suitable according to ignition protection type and the application. Take note of the selection criteria acc. to EN 60079-14.
  - Threads must have no damages.
  - The threads for mounting certified cable entries are of type M20 x 1.5 with sensors of the PROTRAC series (x)xxxTRACxT31/2.DK\*\*\*M\*\*, (x)xxxxTRACxT31.AW\*\*\*M\*\*.
  - The threads for mounting certified cable entries are of type ½-14 NPT with sensors of the PROTRAC series (x)xxxTRAC xT31/2.DK\*\*\*N\*\*, (x)xxxxTRAC xT31.AW\*\*\*N\*\*.

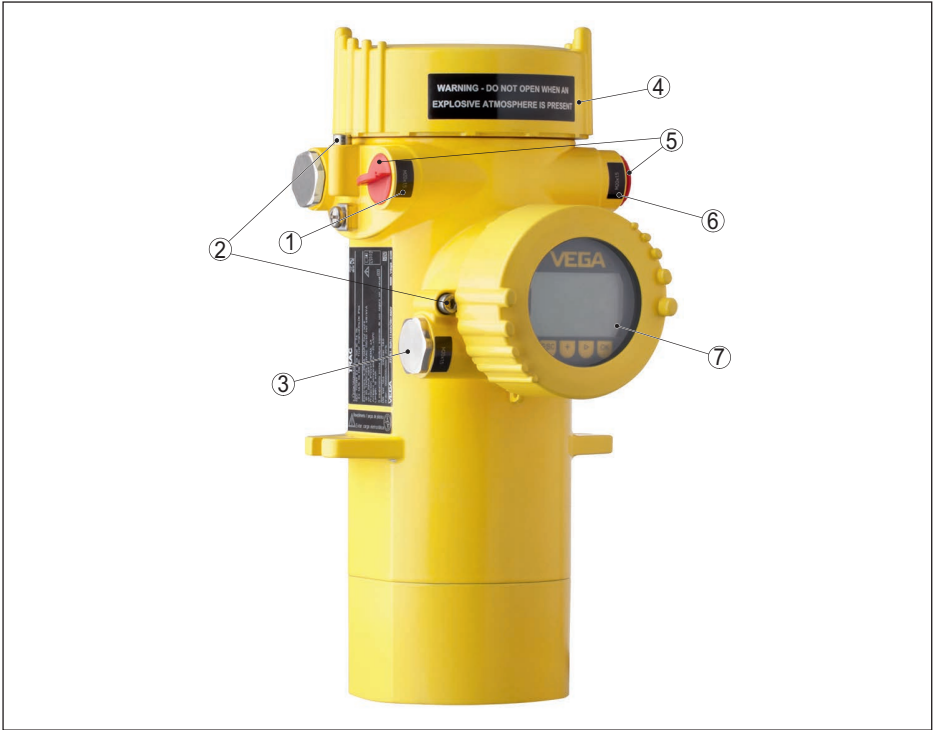

- 1 Label: Type and size of the thread ½-14 NPT or M20 x 1.5
- 2 Locking screw of the lid
- 3 Screw plug
- 4 Ex-b connection compartment
- 5 Red threaded or dust protection cap
- 6 Label: Type and size of the thread ½-14 NPT or M20 x 1.5
- 7 Ex-i connection compartment

- Cable entries and closing screws should be mounted correctly and according to the safety instructions of the manufacturer to ensure the specified ignition protection type. Supplied cable entries or closing screws meet these requirements.
- The red thread or/dust covers screwed in when the instruments are shipped (depending on the version) must be removed before setup and closed by cable entries or closing screws suitable for the ignition protection type.
- When using certified or suitable cable glands, closing screws or plug connections, it is obligatory to observe the appropriate certificates/documents.
- Before operation tighten the housing lid/s up to the stop to ensure the IP protection rating specified on the type label. Lock the lid by unscrewing the locking screw up to the stop. On the double chamber housing, you have to lock both lids.

The housing lids are marked with a warning label.

**WARNING- DO NOT OPEN WHEN AN  
EXPLOSIVE ATMOSPHERE IS PRESENT**

- Unused openings must be provided with plugs suitable for the ignition protection type. Supplied plugs meet these requirements.

## 4 Installation, assignment zones/EPL areas

### Category 2G instrument (EPL Gb instrument)

The sensors of PROTRAC-Serie (x)xxxTRAC xT31/2.DK\*C/D/E/G\*\*\*\*, (x)xxxxTRAC xT31.AW\*E/G\*\*\*\* are installed in hazardous areas requiring an instrument of category 2G (EPL Gb).

### Category 1D instrument (EPL Da instrument)

The sensors of PROTRAC-Serie (x)xxxTRAC xT31/2.DK\*C/D/E/G\*\*\*\*, (x)xxxxTRAC xT31.AW\*E/G\*\*\*\* are installed in hazardous areas requiring an instrument of category 2D (EPL Db).

### Category 2D instrument (EPL Db instrument)

The sensors of PROTRAC-Serie (x)xxxTRAC xT31/2.DK\*C/D/E/G\*\*\*\*, (x)xxxxTRAC xT31.AW\*E/G\*\*\*\* are installed in hazardous areas requiring an instrument of category 2D (EPL Db).

## 5 Safe operating mode

Do not operate the instrument outside the electrical, thermal and mechanical specifications of the manufacturer.

The supplied cable entries and closing screws are suitable for the specified housing temperature range. If other cable entries and closing screws are used, they will probably specify the permissible ambient temperature on the housing.

To exclude the danger of mechanical damage, the FIBERTRAC FT31/2.DK\*C/D/E/G\*\*\*\*(\*)\*\*, FIBERTRAC FT31.AW\*E/G\*\*\*\*(\*)\*\* must be installed in such a way that the flexible detector is protected from environmental influences.

## 6 Grounding

For safety reasons, the the sensors of PROTRAC-Serie (x)xxxTRAC xT31/2.DK\*C/D/E/G\*\*\*\*, (x)xxxxTRAC xT31.AW\*E/G\*\*\*\* **must be grounded**. The external or internal ground connection terminal on the housing is used for this purpose.

## 7 Material resistance


The sensors of PROTRAC-Serie (x)xxxTRAC xT31/2.DK\*C/D/E/G\*\*\*\*, (x)xxxxTRAC xT31.AW\*E/G\*\*\*\* must only be used in media against which the materials of the wetted parts are sufficiently resistant.

## 8 Different ignition protection types

The sensors can be either used in explosive dust atmospheres or in explosive gas atmospheres.

The operator must specify the selected ignition protection type before installation. The selected ignition protection must be marked by scratching off on the identification mark of the type label.



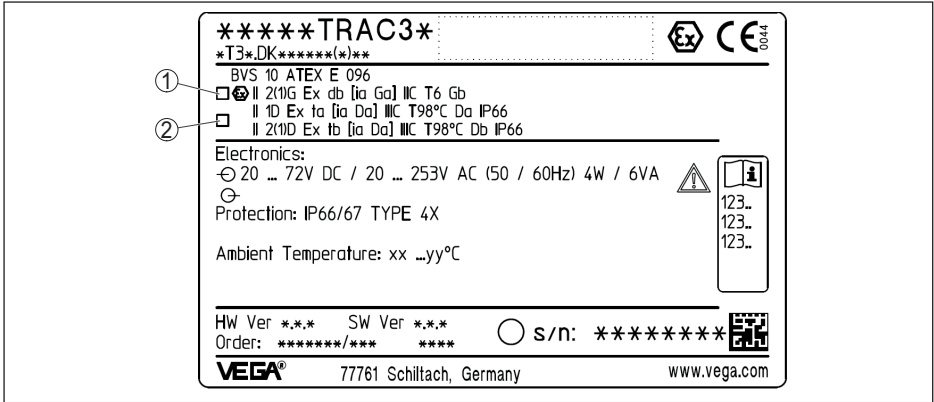

- 1 Identification label Ex-d ignition protection type
- 2 Identification label Ex-t ignition protection type

## 9 Electrical data

### Non-intrinsically safe circuits (in the "Ex-d" connection compartment)

#### PROTRAC-Serie (x)xxxTRAC xT31/2.DK\*C/D/E/G\*\*\*\*, (x)xxxTRAC xT31.AW\*E/G\*\*\*\*

Voltage supply: (terminals 1[L1], 2[N]) U = 20 ... 253 V AC

U = 20 ... 72 V DC

U<sub>m</sub> = 253 V

Relay circuit: (terminals 4[NC], 5[Common], 6[NO]) Maximum values:

253 V AC, 3 A, 500 VA

253 V AC, 1 A, 41 W

Current input: (terminals 12[In+], 13[In-]) I = 4 ... 20 mA

Digital input: (terminals 14[+100 mA], 15[+10 mA], 16[Common])

Digital output: (terminals 17[Out+], 18[Out-])

– Max. load current: floating transistor output 400 mA, 55 V DC

Multigauge Communication: (terminals 19[Serial out-], 20[Serial out+], 21[Serial in-], 22[Serial in+]) Communication circuit, only for communication with additional PROTRAC instruments

#### PROTRAC-Serie (x)xxxTRAC xT31/2.DK\*C/E\*\*\*\*, (x)xxxTRAC xT31.AW\*E\*\*\*\*

Communication circuit: (terminals 10, 11 [Signal+Power] in the "Ex-d" connection compartment) U = 9 ... 32 V DC

**Intrinsically safe circuits (in the "Ex-i" connection compartment)**

**PROTRAC-Serie (x)xxxTRAC xT31/2.DK\*C/D/E/G\*\*\*\*, (x)xxxxTRAC xT31.AW\*E/G\*\*\*\***

Display and adjustment circuit: (terminals 5, 6, 7, 8 in the lateral chamber)

In ignition protection type intrinsic safety Ex ia IIC, IIIC

For connection to an intrinsically safe circuit of the associated external indicating unit VEGADIS 61/81 (PTB 02 ATEX 2136 X and BVS 05 ATEX E 023).

The rules for the interconnection of intrinsically safe circuits between PROTRAC-Serie (x)xxxTRAC xT31/2.DK\*C/D/E/G\*\*\*\*, (x)xxxxTRAC xT31.AW\*E/G\*\*\*\* and the external indicating unit VEGADIS 61/81 are fulfilled, provided that the total inductance and total capacitance of the connection cable between PROTRAC-Serie (x)xxxTRAC xT31/2.DK\*C/D/E/G\*\*\*\*, (x)xxxxTRAC xT31.AW\*E/G\*\*\*\* and the external indicating unit VEGADIS 61/81  $L_{cable} = 100 \mu\text{H}$  and  $C_{cable} = 3.4 \mu\text{F}$  are not exceeded.

When using the delivered VEGA connection cable between PROTRAC-Serie (x)xxxTRAC xT31/2.DK\*C/D/E/G\*\*\*\*, (x)xxxxTRAC xT31.AW\*E/G\*\*\*\* and the external indicating unit VEGADIS 61/81, the following listed cable inductances  $L_i$  and cable capacitances  $C_i$  must be taken into account with a cable length  $\geq 50 \text{ m}$ .

- $L_i = 0.62 \mu\text{H/m}$
- $C_{i \text{ wire/wire}} = 132 \text{ pF/m}$
- $C_{i \text{ wire/screen}} = 208 \text{ pF/m}$
- $C_{i \text{ screen/screen}} = 192 \text{ pF/m}$

Circuit of the display and adjustment module: (spring contacts in the lateral chamber)

In ignition protection type intrinsic safety Ex ia IIC, IIIC

Only for connection to the display and adjustment module PLICSCOM or if it is ensured that an explosive atmosphere is present, for service purposes on the interface adapter VEGACONNECT (PTB 07 ATEX 2013 X).

## PROTRAC-Serie (x)xxxTRAC xT31/2.DK\*D/G\*\*\*\*, (x)xxxTRAC xT31.AW\*G\*\*\*\*

Intrinsically safe communication circuit:  
(terminals 1, 2 [Signal+Power] in the lateral chamber)

In ignition protection type intrinsic safety Ex ia/ib IIC, IIIC  
Only for connection to a certified, intrinsically safe circuit.

Maximum values:

- $U_i = 17.5 \text{ V}$
- $I_i = 500 \text{ mA}$
- $P_i = 5.5 \text{ W}$

Characteristics: linear

The effective internal capacitance  $C_i$  is negligibly small.

The effective internal inductance is  $L_i \leq 5 \mu\text{H}$

The instrument is suitable for connection to a Fieldbus system according to the FISCO model (EN 60079-11: 2012), e.g. Profibus PA, Foundation Fieldbus.

or

- $U_i = 24 \text{ V}$
- $I_i = 250 \text{ mA}$
- $P_i = 1.2 \text{ W}$

Characteristics: linear

The effective internal capacitance  $C_i$  is negligibly small.

The effective internal inductance is  $L_i \leq 5 \mu\text{H}$

## 10 Thermal data

The max. permissible ambient temperatures depending on the temperature classes are specified in the following tables.

### Category 2G instrument (EPL Gb instrument)

Temperature class	Ambient temperature on the sensor
T6	-40 ... +46 °C
T5, T4, T3, T2, T1	-40 ... +60 °C

### Category 1D or 2D instrument (EPL Da or EPL Db instrument)

The max. surface temperature is limited by a temperature fuse to +98 °C.

The permissible ambient temperature is -40 ... +60 °C.

## 11 Protection against static electricity

The PROTRAC-Serie (x)xxxTRAC xT31/2.DK\*C/D/E/G\*\*\*\*, (x)xxxTRAC xT31.AW\*E/G\*\*\*\* in the version with chargeable plastic parts, as e.g. metal housing with inspection window or plastic detectors, is provided with a caution label referring to the safety measures that must be taken with regard to electrostatic charges during operation.

WARNING- POTENTIAL ELECTROSTATIC CHARGING HAZARD - SEE INSTRUCTIONS

Caution: Plastic parts! Danger of electrostatic charging!

- Avoid friction
- No dry cleaning
- Construction/Installation: The PROTRAC-Serie (x)xxxTRAC xT31/2.DK\*C/D/E/G\*\*\*\*, (x)xxxx-TRAC xT31.AW\*E/G\*\*\*\* must be constructed/installed in such a way that
  - electrostatic charges are ruled out during operation, maintenance and cleaning.
  - process-related electrostatic charges, e.g. by measuring media flowing past, are ruled out

## 12 Impact and friction sparks

When used as category 2G (EPL Gb) instruments, the PROTRAC-Serie (x)xxxTRAC xT31/2.DK\*C/D/E/G\*\*\*\*, (x)xxxxTRAC xT31.AW\*E/G\*\*\*\* in light metal versions (e.g. aluminium/titanium/zircon) must be mounted in such a way that sparks from impact and friction between light metals and steel (except stainless steel, if the presence of rust particles can be excluded) cannot occur.

## 13 Mounting with external display unit VEGADIS 61/81

The intrinsically safe signal circuit between PROTRAC-Serie (x)xxxTRAC xT31/2.DK\*C/D/E/G\*\*\*\*, (x)xxxxTRAC xT31.AW\*E/G\*\*\*\* and the external indicating unit VEGADIS 61 or VEGADIS 81 should be set up without grounding. The required insulation voltage is > 500 V AC. When using VEGA connection cable, this requirement is fulfilled. If grounding of the cable screen is required, it must be carried out according to EN 60079-14 (edition 2014).

### Overvoltage arrester, for the display circuit VEGADIS 61/81

As far as acc. to EN 60079-14, paragraph 16.3 (edition 2014) or other valid standards or regulations, an overvoltage protection is necessary, then a suitable overvoltage arrester must be connected to the display circuit of the instrument.

## 14 Ignition protection type flameproof enclosure Ex "d"

The terminals for connecting the operating voltage or signal circuits are integrated in the terminal compartment with ignition protection type flameproof enclosure "d".

The thread gap between housing and cover is a flameproof gap.

The "Ex-d" connection compartment is provided with a M20 x 1.5 or 1/2-14 NPT thread for connection to a certified "Conduit" system or for mounting a "Ex-d" cable entry certified according to EN 60079-1 (edition 2014). Cable entries of simple construction may not be used. Please take note of section 13.1 and 13.2 of EN 60079-1. When connecting to a "Conduit" system, the associated sealing facility must be located directly on the "Ex-d" connection compartment.

When the sensors of PROTRAC-Serie (x)xxxTRAC xT31/2.DK\*C/D/E/G\*\*\*\*, (x)xxxxTRAC xT31.AW\*E/G\*\*\*\* are delivered, depending on the version, the red threaded or dust protection caps must be removed before installing the device and the openings must be sealed according to the requirements of the ignition protection type and the IP protection type specified on the type label.

When using certified or suitable cable glands, closing screws or plug connections, it is obligatory to observe the appropriate certificates/documents.

The "Ex-d" cable entry and the closing screws must be tightly screwed into the housing.

The cable entry sent with the delivery is suitable for the housing temperature range specified in the PROTRAC-Serie (x)xxxTRAC xT31/2.DK\*C/D/E/G\*\*\*\*, (x)xxxxTRAC xT31.AW\*E/G\*\*\*\* certificate. If a different cable entry is used, the separately certified cable entry/gland or the temperature classes on the electronics determines the max. permissible ambient temperature on the housing.

Before opening the lid of the "Ex-d" terminal compartment or in case it is already open (e. g. during connection or service work), make sure that either the supply cable is completely voltage free or no explosive atmosphere is present.

When wiring the connection line to the "Ex-d" terminal compartment, it must be sufficiently secured against damage and in conformity with EN 60079-14.

The connection cables, the cable entries and the closing screws or the pipeline sealing facilities must be suitable for the lowest ambient temperature.

The cover of the "Ex-d" connection compartment must be screwed in completely before commissioning and secured by screwing out the lid locking screw all the way to the stop.

Unused openings must be sealed according to EN 60079-1 paragraph 13.8 (edition 2014).

The flame path joints must not be repaired.

## Double chamber housing with "Ex-d" connection compartment



- 1 "Ex-i" connection compartment
- 2 Locking screws of the cover
- 3 "Ex-d" connection compartment

## 15 Ignition protection type protection by enclosure Ex "t"

Before setup and application of the PROTRAC-Serie (x)xxxTRAC xT31/2.DK\*C/D/E/G\*\*\*\*, (x)xxxTRAC xT31.AW\*E/G\*\*\*\* as explosion-proof instruments of category 1D (EPL Da) or category 2D (EPL Db) the two lids have to be screwed in to the stop.

When the sensors of PROTRAC-Serie (x)xxxTRAC xT31/2.DK\*C/D/E/G\*\*\*\*, (x)xxxTRAC xT31.AW\*E/G\*\*\*\* are delivered, depending on the version, the red threaded or dust protection caps must be removed before installing the device and the openings must be sealed according to the requirements of the ignition protection type and the IP protection type specified on the type label.

When using certified or suitable cable glands, closing screws or plug connections, it is obligatory to observe the appropriate certificates/documents.

The "Ex-t" cable entry and the closing screws must be tightly screwed into the housing.

Cable entries must only be replaced by the same types or suitable cable entries/glands which are certified according to ATEX with at least IP 66.

The cable entry sent with the delivery is suitable for the housing temperature range specified in the certificate of PROTRAC-Serie (x)xxxTRAC xT31/2.DK°C/D/E/G\*\*\*\*, (x)xxxxTRAC xT31.AW\*E/G\*\*\*\*. If a different cable entry is used, the separately certified cable entry/gland determines the max. permissible ambient temperature on the housing.

## 16 Instructions for zone 20 applications

In hazardous areas, the instrument should only be operated under atmospheric conditions:

- Temperature: -20 ... +60 °C.
- Pressure: 80 ... 110 kPa (0.8 ... 1.1 bar)
- Air with normal oxygen content, normally 21 %

If there are no explosive mixtures, then the instruments can be also operated according to the manufacturer specification outside atmospheric conditions.

If there is a risk of dangerous potential differences inside zone 20, then suitable measures for intrinsically safe circuits in zone 20 must be taken, e.g. according to the requirements of EN 60079-14 section 16.3 (edition 2014).

## 17 Ignition protection type intrinsic safety Ex "ia"

Optionally the VEGA display and adjustment module PLICSCOM can be integrated.

The VEGA display and adjustment unit VEGADIS 61 or VEGADIS 81 (PTB 02 ATEX 2136X) can be connected if necessary. The respective operating or safety instructions must be observed.

The VEGA interface adapter VEGACONNECT (PTB 07 ATEX 2013 X) can be connected for service purposes. The respective operating or safety instructions must be observed. Intrinsic safety proofs are not necessary.

The PROTRAC-Serie (x)xxxTRAC xT31/2.DK°C/D/E/G\*\*\*\*, (x)xxxxTRAC xT31.AW\*E/G\*\*\*\* has an intrinsically safe current output.

Only connect the instrument to certified associated instruments with protective level Ex ia (EPL Ga) or Ex ib (EPL Gb). When connecting to an associated instrument with protective level Ex ib (EPL Gb), then the flame proofing changes to Ex ib. After the use as EPL Gb instrument with Ex-ib supply, the use as EPL Ga instrument is no longer permitted.

The regulations for connection of intrinsically safe circuits (e.g. EN 60079-14, proof of intrinsic safety) must be observed

The intrinsically safe output circuits are ground-free. The voltage resistance is min. 500 Veff against ground.

## 18 Use of an overvoltage arrester

If necessary, a suitable overvoltage arrester can be connected in front of the sensors of PROTRAC-Serie (x)xxxTRAC xT31/2.DK°C/D/E/G\*\*\*\*, (x)xxxxTRAC xT31.AW\*E/G\*\*\*\*.

As far as acc. to EN 60079-14, paragraph 16.3 (edition 2014) or other valid standards or regulations, an overvoltage protection is necessary, then a suitable overvoltage arrester must be connected to the instrument.

Observe the respective operating or safety instructions.

## 19 Version with cooling option

With sensors of PROTRAC-Serie (x)xxxTRAC xT31/2.DK\*C/D/E/G\*\*\*\*, (x)xxxTRAC xT31. AW\*E/G\*\*\*\* with optional accessory of the cooling option, the operator must take care that the approved ambient temperature range on the Ex-certified housing, electronics is not exceeded.

Please make sure that before cooling, there is no explosive atmosphere present in the cooling option.

Printing date:

# VEGA

All statements concerning scope of delivery, application, practical use and operating conditions of the sensors and processing systems correspond to the information available at the time of printing.

Subject to change without prior notice

© VEGA Grieshaber KG, Schiltach/Germany 2017



55440-EN-171221

VEGA Grieshaber KG  
Am Hohenstein 113  
77761 Schiltach  
Germany

Phone +49 7836 50-0  
Fax +49 7836 50-201  
E-mail: [info.de@vega.com](mailto:info.de@vega.com)  
[www.vega.com](http://www.vega.com)