

Safety instructions
CCOE approval
FIBERTRAC 31, 32
SOLITRAC 31
MINITRAC 31, 32
POINTRAC 31
WEIGHTRAC 31, 32

Flameproof enclosures
Intrinsic safety
P445283/1
Profibus PA
Foundation Fieldbus



Document ID: 63113



VEGA

Contents

1	Area of applicability.....	3
2	General information.....	3
3	Special instructions for installation.....	5
4	Installation, assignment zones/EPL areas.....	7
5	Safe operating mode.....	7
6	Grounding.....	7
7	Material resistance.....	7
8	Electrical data.....	7
9	Thermal data.....	9
10	Protection against static electricity.....	9
11	Impact and friction sparks.....	10
12	Mounting with external display unit VEGADIS 61/81.....	10
13	Type of protection flameproof enclosure Ex "d".....	10
14	Type of protection intrinsic safety Ex "ia".....	11
15	Use of an overvoltage arrester.....	12
16	Version with cooling option.....	12
17	Electrostatic charging (ESD).....	12

Supplementary documentation:

- Operating Instructions FIBERTRAC 31, 32, SOLITRAC 31, MINITRAC 31, 32, POINTRAC 31, WEIGHTRAC 31, 32
- Letter P445283/1 By Government of India (Document ID: 63114)

Editing status: 2019-11-22

1 Area of applicability

These safety instructions apply to the radiometric sensors of the PROTRAC series:

FIBERTRAC FT3*.****(*)*

SOLITRAC ST3*.****(*)**

MINITRAC MT3*.****

POINTRAC PT3*.****(*)**

WEIGHTRAC WT3*.****

according to Letter P445283/1 By Government of India (certificate number on the type label) and for all instruments with safety instruction 63113.

2 General information

The sensors of the PROTRAC series are part of the radiometric measuring principle.

In a radiometric measurement, a weak radioactive source on the tank emits focused gamma rays. A special detector mounted on the opposite side of the tank receives the radiation which is converted into flashes of light. The number of these flashes is detected and evaluated.

The FIBERTRAC 31, FIBERTRAC 32 and SOLITRAC 31 sensors of the PROTRAC series are suitable for non-contact level and interface measurement.

The MINITRAC 31, MINITRAC 32 sensors of the PROTRAC series are suitable for the non-contact, continuous density measurement and level detection of liquids and bulk solids in pipelines and vessels.

The POINTRAC 31 sensors of the PROTRAC series are suitable for non-contact level detection of liquids and bulk solids.

The WEIGHTRAC 31, WEIGHTRAC 32 sensors of the PROTRAC series are suitable for non-contact, continuous mass flow measurement of bulk solids on conveyor belts and screw conveyors.

The sensors of the PROTRAC series FIBERTRAC FT31/2.DK*C/D/E/G****(*)**, FIBERTRAC FT31.AW*E/G****(*)**, SOLITRAC ST31.DK*C/D/E/G****(*)**, SOLITRAC ST31.AW*E/G****(*)**, MINITRAC MT31/2.DK*C/D/E/G****, MINITRAC MT31.AW*E/G****, POINTRAC PT31.DK*C/D/E/G****(*)**, POINTRAC PT31.AW*E/G****(*)**, WEIGHTRAC WT31/2.DK*C/D/E/G**** when used with "Flameproof enclosure (Ex d)" are suitable for the use in hazardous atmosphere of all combustible substances of explosion groups IIA, IIB and IIC, for applications requiring instruments of category 2G.

The sensors of the PROTRAC series are suitable for applications requiring category 2G (EPL Gb) instruments.

If the PROTRAC-Serie (x)xxxTRAC xT31/2.DK*C/D/E/G****, (x)xxxxTRAC xT31.AW*E/G**** are installed and operated in hazardous areas, the general Ex installation regulations EN 60079-14 as well as these safety instructions must be observed.

Type of protection marking

EN 60079-0: 2012/A11: 2013

EN 60079-1: 2014

EN 60079-11: 2012

Ex db [ia Ga] IIC T6 Gb

Important specification in the type code

PROTRAC-Serie (x)xxxxTRAC xT3*.a*cdef*h(*)

Position		Feature	Description
(x)xxxxTRAC	Device name	FIBER	FIBERTRAC FT31, FIBERTRAC FT32
		SOLI	SOLITRAC ST31
		MINI	MINITRAC MT31, MINITRAC MT32
		POIN	POINTRAC PT31
		WEIGH	WEIGHTRAC WT31, WEIGHTRAC WT32
xT3*	Instrument code	F	FIBERTRAC FT31, FIBERTRAC FT32
		S	SOLITRAC ST31
		M	MINITRAC MT31, MINITRAC MT32
		P	POINTRAC PT31
		W	WEIGHTRAC WT31, WEIGHTRAC WT32
a	Approval	DK	Ex db [ia Ga] IIC T6 Gb
c	Electronics	C	Four-wire, Foundation Fieldbus (Ex-d output)
		D	Four-wire, Foundation Fieldbus (Ex-ia output)
		E	Four-wire, Profibus PA (Ex-d output)
		G	Four-wire, Profibus PA (Ex-ia output)
d	Housing / Protection	D	Aluminium double chamber / IP66/IP67
		W	Stainless steel double chamber / IP66/IP67
		A	Aluminium double chamber with 316L Conduit cooling connection / IP66/IP67
		V	Stainless steel double chamber with 316L Conduit cooling connection / IP66/IP67
		S	Aluminium double chamber (special colour) / IP66/IP67
		R	Aluminium double chamber (special colour) with 316L Conduit cooling connection / IP66/IP67
e	Cable entry / Cable gland / Plug connection	M	M20 x 1.5 / without / without
		N	½ NPT / without / without
f	Display and adjustment module PLICSCOM	X	without
		F	without; lid with inspection window
		B	Laterally mounted
		L	laterally mounted; with Bluetooth, magnetic pen operation
		S	laterally mounted; with Bluetooth, battery, magnetic pen operation
h	Measuring length	(*)**	2 or 3-digit measuring length of the sensor connection with FIBERTRAC FT31, FIBERTRAC FT32, SOLITRAC ST31 and POINTRAC PT31 This feature is not available with MINITRAC MT31, MINITRAC MT32.

Position		Feature	Description
h(*)	Frame setup	***	Different features of the frame setup with frame construction, measuring width, clear height and source fastening with WEIGHTRAC WT31, WEIGHTRAC WT32

3 Special instructions for installation

- The following requirements must be fulfilled for mounting, electrical installation, setup and maintenance of the instrument:
 - The staff must be qualified according the respective tasks
 - The staff must be trained in explosion protection
 - The staff must be familiar with the respectively valid regulations, e.g. planning and installation acc. to EN 60079-14
- The instrument has to be mounted according to the manufacturer specifications and the valid regulations and standards.
- Modifications on the instruments can influence the explosion protection and hence the safety. Modifications must only be carried out by employees authorized by VEGA company.
- Keep in mind for instrument mounting
 - mechanical damage on the instrument must be avoided
 - mechanical friction must be avoided
- The instruments must be mounted/installed in such a way that the following can be ruled out:
 - electrostatic charges during operation, maintenance and cleaning.
 - process-related electrostatic charges, e.g. by measuring media flowing past
- Take note of the type and size of the thread
 - Label in the area of the thread with respective name.
 - Only use the cable entries and closing screws if they are required and suitable according to ignition protection type and the application. Take note of the selection criteria acc. to EN 60079-14.
 - Threads must have no damages.
 - The threads for mounting certified cable entries are of type M20 x 1.5 with sensors of the PROTRAC series (x)xxxTRACxT31/2.DK***M**, (x)xxxxTRACxT31.AW***M**.
 - The threads for mounting certified cable entries are of type ½-14 NPT with sensors of the PROTRAC series (x)xxxTRAC xT31/2.DK****N**, (x)xxxxTRAC xT31.AW****N**.



- 1 Label: Type and size of the thread ½-14 NPT or M20 x 1.5
- 2 Locking screw of the lid
- 3 Screw plug
- 4 Ex-b connection compartment
- 5 Red threaded or dust protection cap
- 6 Label: Type and size of the thread ½-14 NPT or M20 x 1.5
- 7 Ex-i connection compartment

- Cable entries and closing screws should be mounted correctly and according to the safety instructions of the manufacturer to ensure the specified ignition protection type. Supplied cable entries or closing screws meet these requirements.
- The red thread or/dust covers screwed in when the instruments are shipped (depending on the version) must be removed before setup and closed by cable entries or closing screws suitable for the ignition protection type.
- When using certified or suitable cable glands, closing screws or plug connections, it is obligatory to observe the appropriate certificates/documents.
- Before operation tighten the housing lid/s up to the stop to ensure the IP protection rating specified on the type label. Lock the lid by unscrewing the locking screw up to the stop. On the double chamber housing, you have to lock both lids.

The housing lids are marked with a warning label.

WARNING - DO NOT OPEN WHEN AN
EXPLOSIVE ATMOSPHERE IS PRESENT

- Unused openings must be provided with plugs suitable for the ignition protection type. Supplied plugs meet these requirements.

4 Installation, assignment zones/EPL areas

Category 2G instrument (EPL Gb instrument)

The sensors of PROTRAC-Serie (x)xxxTRAC xT31/2.DK*C/D/E/G****, (x)xxxxTRAC xT31.AW*E/G**** are installed in hazardous areas requiring an instrument of category 2G (EPL Gb).

5 Safe operating mode

Do not operate the instrument outside the electrical, thermal and mechanical specifications of the manufacturer.

The supplied cable entries and closing screws are suitable for the specified housing temperature range. If other cable entries and closing screws are used, they will probably specify the permissible ambient temperature on the housing.

To exclude the danger of mechanical damage, the FIBERTRAC FT31/2.DK*C/D/E/G****(*)**, FIBERTRAC FT31.AW*E/G****(*)** must be installed in such a way that the flexible detector is protected from environmental influences.

6 Grounding

For safety reasons, the the sensors of PROTRAC-Serie (x)xxxTRAC xT31/2.DK*C/D/E/G****, (x)xxxxTRAC xT31.AW*E/G**** must be grounded. The external or internal ground connection terminal on the housing is used for this purpose.

7 Material resistance

The sensors of PROTRAC-Serie (x)xxxTRAC xT31/2.DK*C/D/E/G****, (x)xxxxTRAC xT31.AW*E/G**** must only be used in media against which the materials of the wetted parts are sufficiently resistant.

8 Electrical data

Non-intrinsically safe circuits (in the "Ex-d" connection compartment)

PROTRAC-Serie (x)xxxTRAC xT31/2.DK*C/D/E/G****, (x)xxxxTRAC xT31.AW*E/G****

Voltage supply: (terminals 1[L1], 2[N])	U = 20 ... 253 V AC
	U = 20 ... 72 V DC
	U _m = 253 V
Relay circuit: (terminals 4[NC], 5[Common], 6[NO])	Maximum values: 253 V AC, 3 A, 500 VA 253 V AC, 1 A, 41 W
Current input: (terminals 12[In+], 13[In-])	I = 4 ... 20 mA
Digital input: (terminals 14[+100 mA], 15[+10 mA], 16[Common])	
Digital output: (terminals 17[Out+], 18[Out-])	
– Max. load current: floating transistor output	400 mA, 55 V DC

Multigauge Communication: (terminals 19[Serial out-], 20[Serial out+], 21[Serial in-], 22[Serial in+]) Communication circuit, only for communication with additional PROTRAC instruments

PROTRAC-Serie (x)xxxxTRAC xT31/2.DK*C/E**, (x)xxxxTRAC xT31.AW*E******

Communication circuit: (terminals 10, 11 U= 9 ... 32 V DC [Signal+Power] in the "Ex-d" connection compartment)

Intrinsically safe circuits (in the "Ex-i" connection compartment)

PROTRAC-Serie (x)xxxTRAC xT31/2.DK*C/D/E/G**, (x)xxxxTRAC xT31.AW*E/G******

Display and adjustment circuit: (terminals 5, 6, 7, 8 in the lateral chamber) In type of protection intrinsic safety Ex ia IIC, IIIC

For connection to an intrinsically safe circuit of the associated external indicating unit VEGADIS 61/81 (PTB 02 ATEX 2136 X and BVS 05 ATEX E 023).

The rules for the interconnection of intrinsically safe circuits between PROTRAC-Serie (x)xxxTRAC xT31/2.DK*C/D/E/G****, (x)xxxxTRAC xT31.AW*E/G**** and the external indicating unit VEGADIS 61/81 are fulfilled, provided that the total inductance and total capacitance of the connection cable between PROTRAC-Serie (x)xxxTRAC xT31/2.DK*C/D/E/G****, (x)xxxxTRAC xT31.AW*E/G**** and the external indicating unit VEGADIS 61/81 $L_{cable} = 100 \mu H$ and $C_{cable} = 3.4 \mu F$ are not exceeded.

When using the delivered VEGA connection cable between PROTRAC-Serie (x)xxxTRAC xT31/2.DK*C/D/E/G****, (x)xxxxTRAC xT31.AW*E/G**** and the external indicating unit VEGADIS 61/81, the following listed cable inductances L_i and cable capacitances C_i must be taken into account with a cable length ≥ 50 m.

- $L_i = 0.62 \mu H/m$
- $C_{i \text{ wire/wire}} = 132 \text{ pF/m}$
- $C_{i \text{ wire/screen}} = 208 \text{ pF/m}$
- $C_{i \text{ screen/screen}} = 192 \text{ pF/m}$

Circuit of the display and adjustment module: (spring contacts in the lateral chamber)

In type of protection intrinsic safety Ex ia IIC, IIIC

Only for connection to the display and adjustment module PLICSCOM or if it is ensured that on explosive atmosphere is present, for service purposes on the interface adapter VEGACONNECT (PTB 07 ATEX 2013 X).

The intrinsically safe display/control circuit is earthed and connected to the external and internal earth terminal.

PROTRAC-Serie (x)xxxxTRAC xT31/2.DK*D/G****, (x)xxxxTRAC xT31.AW*G****

Intrinsically safe communication circuit:
(terminals 1, 2 [Signal+Power] in the lateral chamber)

In type of protection intrinsic safety Ex ia/ib IIC, IIIC

Only for connection to a certified, intrinsically safe circuit.

Maximum values:

- $U_i = 17.5 \text{ V}$
- $I_i = 500 \text{ mA}$
- $P_i = 5.5 \text{ W}$

Characteristics: Linear

The effective internal capacitance C_i is negligibly small.

The effective internal inductance is $L_i \leq 5 \mu\text{H}$

The instrument is suitable for connection to a Fieldbus system according to the FISCO model (EN 60079-11: 2012), e.g. Profibus PA, Foundation Fieldbus.

or

- $U_i = 24 \text{ V}$
- $I_i = 250 \text{ mA}$
- $P_i = 1.2 \text{ W}$

Characteristics: Linear

The effective internal capacitance C_i is negligibly small.

The effective internal inductance is $L_i \leq 5 \mu\text{H}$

9 Thermal data

The max. permissible ambient temperatures depending on the temperature classes are specified in the following tables.

Category 2G instrument (EPL Gb instrument)

Temperature class	Ambient temperature on the sensor
T6	-40 ... +46 °C
T5, T4, T3, T2, T1	-40 ... +60 °C

10 Protection against static electricity

The PROTRAC-Serie (x)xxxTRAC xT31/2.DK*C/D/E/G****, (x)xxxxTRAC xT31.AW*E/G**** in the version with chargeable plastic parts, as e.g. metal housing with inspection window or plastic detectors, is provided with a caution label referring to the safety measures that must be taken with regard to electrostatic charges during operation.

WARNING - POTENTIAL ELECTROSTATIC CHARGING HAZARD - SEE INSTRUCTIONS

Caution: Plastic parts! Danger of electrostatic charging!

- Avoid friction
- No dry cleaning
- Construction/Installation: The PROTRAC-Serie (x)xxxTRAC xT31/2.DK*C/D/E/G****, (x)xxxx-TRAC xT31.AW*E/G**** must be constructed/installed in such a way that

- electrostatic charges are ruled out during operation, maintenance and cleaning.
- process-related electrostatic charges, e.g. by measuring media flowing past, are ruled out

11 Impact and friction sparks

When used as category 2G (EPL Gb) instruments, the PROTRAC-Serie (x)xxxTRAC xT31/2.DK°C/D/E/G****, (x)xxxxTRAC xT31.AW*E/G**** in light metal versions (e.g. aluminium/titanium/zircon) must be mounted in such a way that sparks from impact and friction between light metals and steel (except stainless steel, if the presence of rust particles can be excluded) cannot occur.

12 Mounting with external display unit VEGADIS 61/81

The intrinsically safe signal circuit between PROTRAC-Serie (x)xxxTRAC xT31/2.DK°C/D/E/G****, (x)xxxxTRAC xT31.AW*E/G**** and the external indicating unit VEGADIS 61 or VEGADIS 81 should be set up without grounding. The required insulation voltage is > 500 V AC. When using VEGA connection cable, this requirement is fulfilled. If grounding of the cable screen is required, it must be carried out according to EN 60079-14 (edition 2014).

Overvoltage arrester, for the display circuit VEGADIS 61/81

As far as acc. to EN 60079-14, paragraph 16.3 (edition 2014) or other valid standards or regulations, an overvoltage protection is necessary, then a suitable overvoltage arrester must be connected to the display circuit of the instrument.

13 Type of protection flameproof enclosure Ex "d"

The terminals for connecting the operating voltage or signal circuits are integrated in the connection compartment with type of protection flameproof enclosure "d".

The thread gap between housing and cover is a flameproof gap.

The "Ex-d" connection compartment is provided with a M20 x 1.5 or ½-14 NPT thread for connection to a certified "Conduit" system or for mounting a "Ex-d" cable entry certified according to EN 60079-1 (edition 2014). Cable entries of simple construction may not be used. Please take note of section 13.1 and 13.2 of EN 60079-1. When connecting to a "Conduit" system, the associated sealing facility must be located directly on the "Ex-d" connection compartment.

When the sensors of PROTRAC-Serie (x)xxxTRAC xT31/2.DK°C/D/E/G****, (x)xxxxTRAC xT31.AW*E/G**** are delivered, depending on the version, the red threaded or dust protection caps must be removed before installing the device and the openings must be sealed according to the requirements of the type of protection and the IP protection type specified on the type label.

When using certified or suitable cable glands, closing screws or plug connections, it is obligatory to observe the appropriate certificates/documents.

The "Ex-d" cable entry and the closing screws must be tightly screwed into the housing.

The cable entry sent with the delivery is suitable for the housing temperature range specified in the PROTRAC-Serie (x)xxxTRAC xT31/2.DK°C/D/E/G****, (x)xxxxTRAC xT31.AW*E/G**** certificate. If a different cable entry is used, the separately certified cable entry/gland or the temperature classes on the electronics determines the max. permissible ambient temperature on the housing.

Before opening the lid of the "Ex-d" terminal compartment or in case it is already open (e. g. during connection or service work), make sure that either the supply cable is completely voltage free or no explosive atmosphere is present.

When wiring the connection line to the "Ex-d" terminal compartment, it must be sufficiently secured against damage and in conformity with EN 60079-14.

The connection cables, the cable entries and the closing screws or the pipeline sealing facilities must be suitable for the lowest ambient temperature.

The cover of the "Ex-d" connection compartment must be screwed in completely before commissioning and secured by screwing out the lid locking screw all the way to the stop.

Unused openings must be sealed according to EN 60079-1 paragraph 13.8 (edition 2014).

The flame path joints must not be repaired.

Double chamber housing with "Ex-d" connection compartment



- 1 "Ex-i" connection compartment
- 2 Locking screws of the cover
- 3 "Ex-d" connection compartment

14 Type of protection intrinsic safety Ex "ia"

Optionally the VEGA display and adjustment module PLICSCOM can be integrated.

The VEGA display and adjustment unit VEGADIS 61 or VEGADIS 81 (PTB 02 ATEX 2136X) can be connected if necessary. The respective operating or safety instructions must be observed.

The VEGA interface adapter VEGACONNECT (PTB 07 ATEX 2013 X) can be connected for service purposes. The respective operating or safety instructions must be observed. Intrinsic safety proofs are not necessary.

The PROTRAC-Serie (x)xxxTRAC xT31/2.DK*C/D/E/G****, (x)xxxTRAC xT31.AW*E/G**** has an intrinsically safe current output.

Only connect the instrument to certified associated instruments with protective level Ex ia (EPL Ga) or Ex ib (EPL Gb). When connecting to an associated instrument with protective level Ex ib

(EPL Gb), then the flame proofing changes to Ex ib. After the use as EPL Gb instrument with Ex-ib supply, the use as EPL Ga instrument is no longer permitted.

The regulations for connection of intrinsically safe circuits (e.g. EN 60079-14, proof of intrinsic safety) must be observed

The intrinsically safe output circuits are ground-free. The voltage resistance is min. 500 Veff against ground.

15 Use of an overvoltage arrester

If necessary, a suitable overvoltage arrester can be connected in front of the sensors of PROTRAC-Serie (x)xxxTRAC xT31/2.DK*C/D/E/G****, (x)xxxxTRAC xT31.AW*E/G****.

As far as acc. to EN 60079-14, paragraph 16.3 (edition 2014) or other valid standards or regulations, an overvoltage protection is necessary, then a suitable overvoltage arrester must be connected to the instrument.

Observe the respective operating or safety instructions.

16 Version with cooling option

With sensors of PROTRAC-Serie (x)xxxTRAC xT31/2.DK*C/D/E/G****, (x)xxxxTRAC xT31.AW*E/G**** with optional accessory of the cooling option, the operator must take care that the approved ambient temperature range on the Ex-certified housing, electronics is not exceeded.

Please make sure that before cooling, there is no explosive atmosphere present in the cooling option.

17 Electrostatic charging (ESD)

In case of instrument versions with electrostatically chargeable plastic parts, the danger of electrostatic charging and discharging must be taken into account!

The following parts can charge and discharge:

- Lacquered housing version or alternative special lacquering
- Plastic housing, plastic housing parts
- Metal housing with inspection window
- Plastic process fittings
- Plastic-coated process fittings and/or plastic-coated sensors
- Connection cable for separate versions
- Type label
- Isolated metallic labels (measuring point identification plate)

Take note in case of danger of electrostatic charges:

- Avoid friction on the surfaces
- Do not dry clean the surfaces

The instruments must be mounted/installed in such a way that the following can be ruled out:

- electrostatic charges during operation, maintenance and cleaning.
- process-related electrostatic charges, e.g. by measuring media flowing past


The warning label indicates danger:

WARNING - POTENTIAL ELECTROSTATIC CHARGING HAZARD - SEE INSTRUCTIONS

Confirmation

Hereby the company VEGA Grieshaber KG declares that the approved CCOE devices have been manufactured in accordance with the ATEX approval mentioned in the attached CCOE certificate.

VEGA Grieshaber KG
A m H o h e n s t e i n 1 1 3
7 7 7 6 1 S c h i l t a c h / G e r m a n y
T e l . + 4 9 7 8 3 6 5 0 - 0
E-mail: info@vega.com - www.vega.com

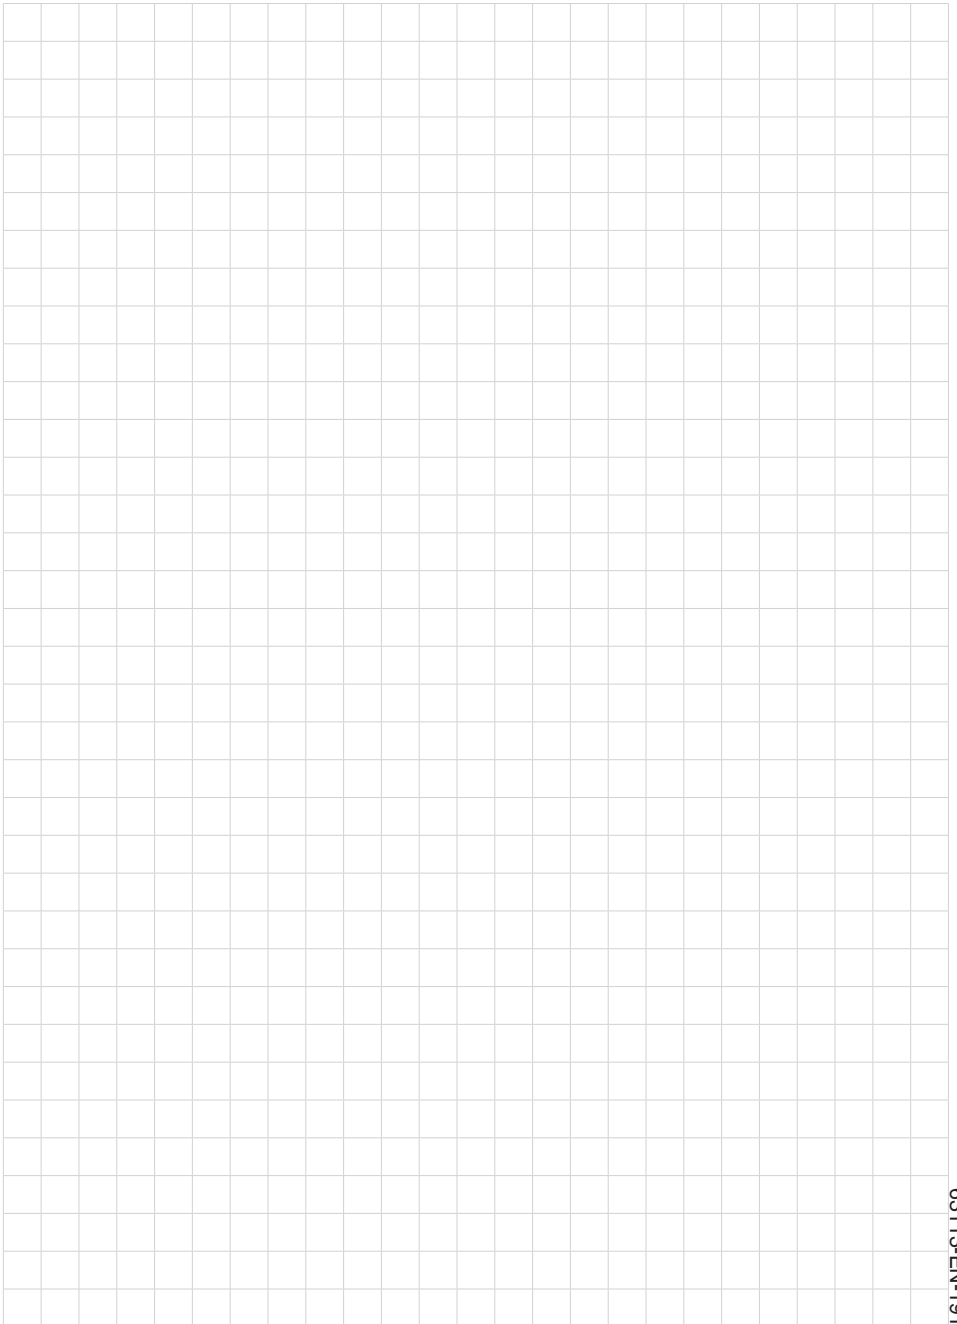



Printing date:

VEGA

All statements concerning scope of delivery, application, practical use and operating conditions of the sensors and processing systems correspond to the information available at the time of printing.

Subject to change without prior notice

© VEGA Grieshaber KG, Schiltach/Germany 2019

63113-EN-191126

VEGA Grieshaber KG
Am Hohenstein 113
77761 Schiltach
Germany

Phone +49 7836 50-0
Fax +49 7836 50-201
E-mail: info.de@vega.com
www.vega.com